



New 100 488,561,633,405

| | | | |
|-------------------|-----------|--------------|-----------------------|
| Cytometer: | FACSriaII | User: | BDSservice |
| Cytometer Name: | FACSriaII | Institution: | |
| Serial Number: | 1 | Software: | BD FACSDiva 6.1.3 |
| Input Device: | Manual | Date: | 7/31/2013 10:36:47 AM |
| Sheath Pressure: | 17.00 | | |
| Nozzle Size: | 100 | | |
| Window Extension: | 2.00 | | |


Red Laser (633nm)

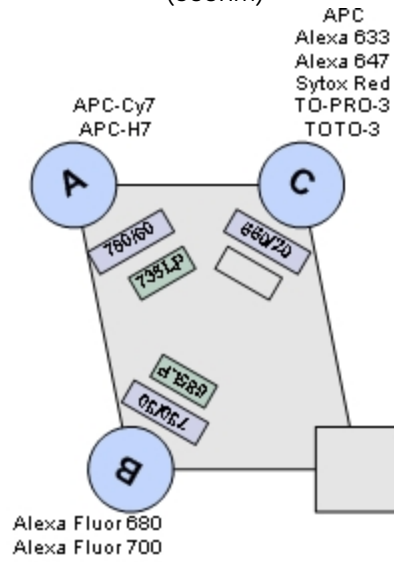


Yellow Green Laser
(561nm)

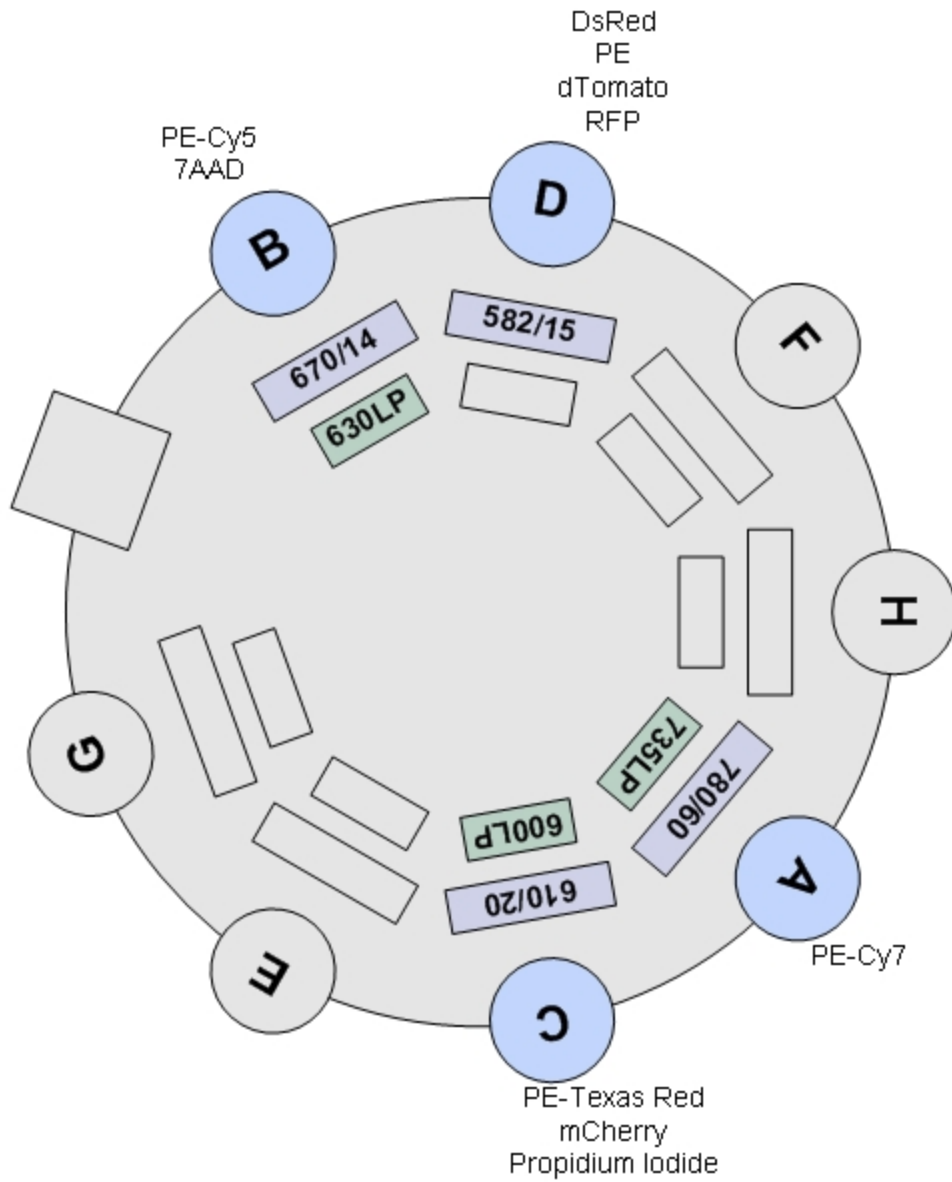

Blue Laser
(488nm)
SSC

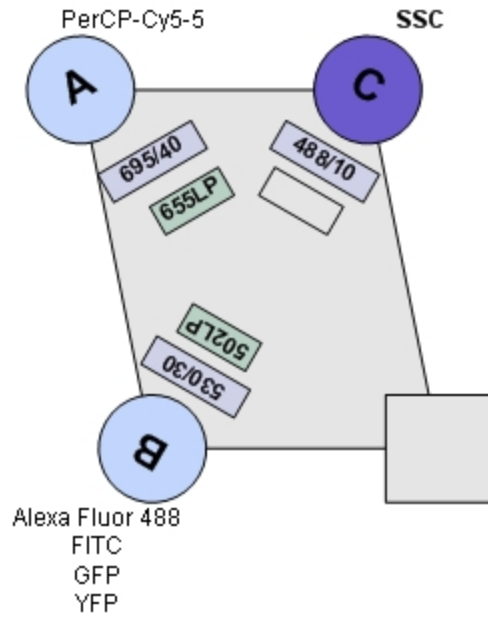

Violet Laser
(407nm)

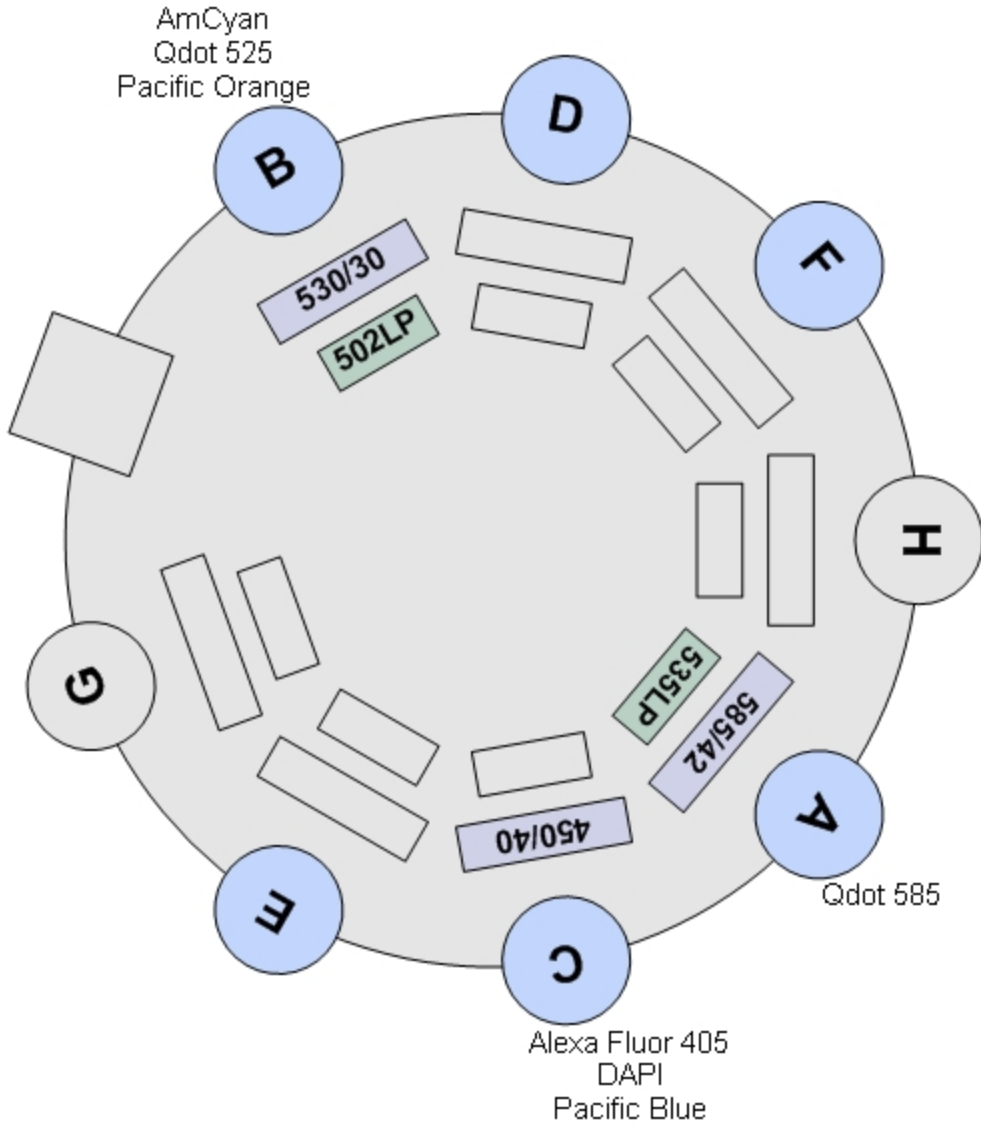

Comments: