



New 100 488,561,633,405

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	3/14/2013 1:56:14 PM
Sheath Pressure:	17.00		
Nozzle Size:	100		
Window Extension:	2.00		


Red Laser (633nm)

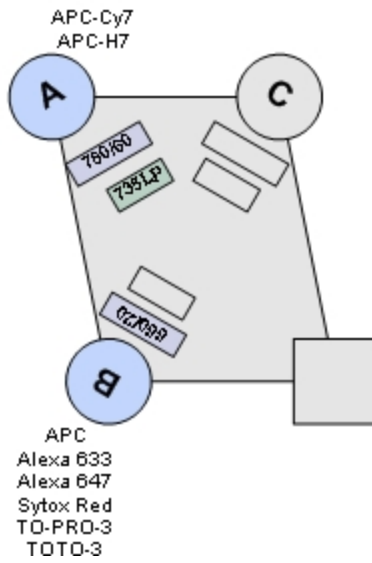

Yellow Green Laser
(561nm)

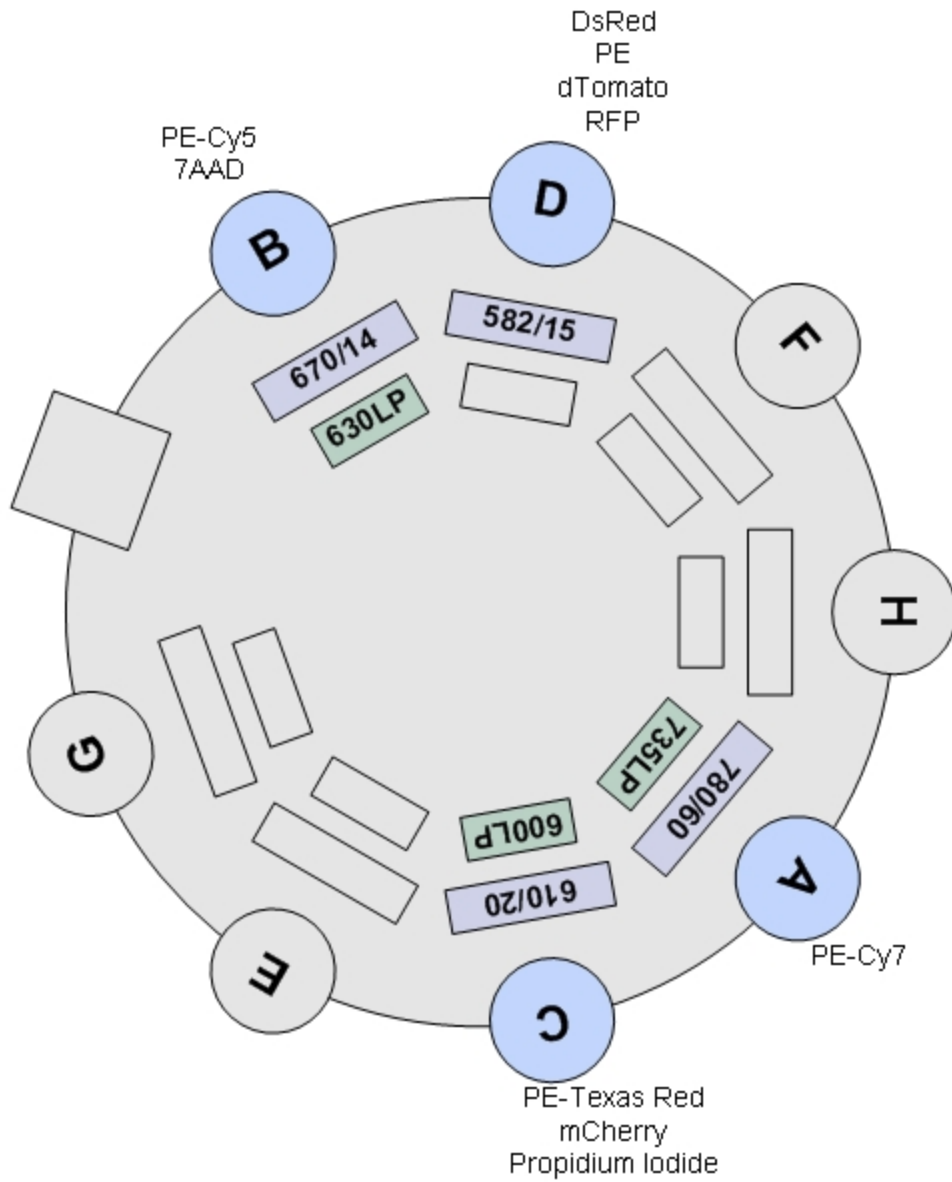


Blue Laser
(488nm)
SSC

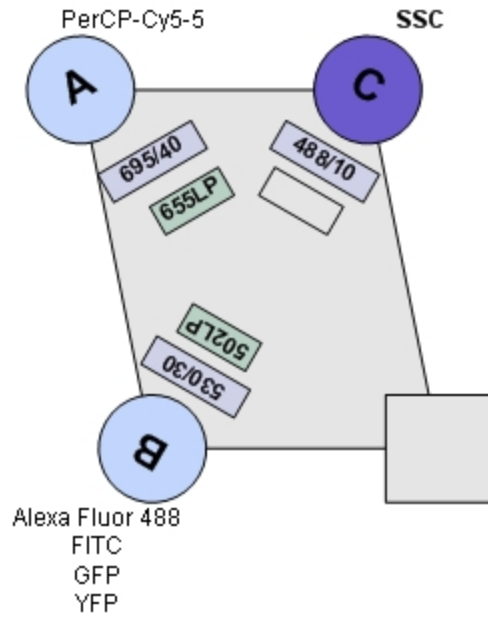

Violet Laser
(407nm)

Alexa Fluor 405
DAPI
Pacific Blue
V 450

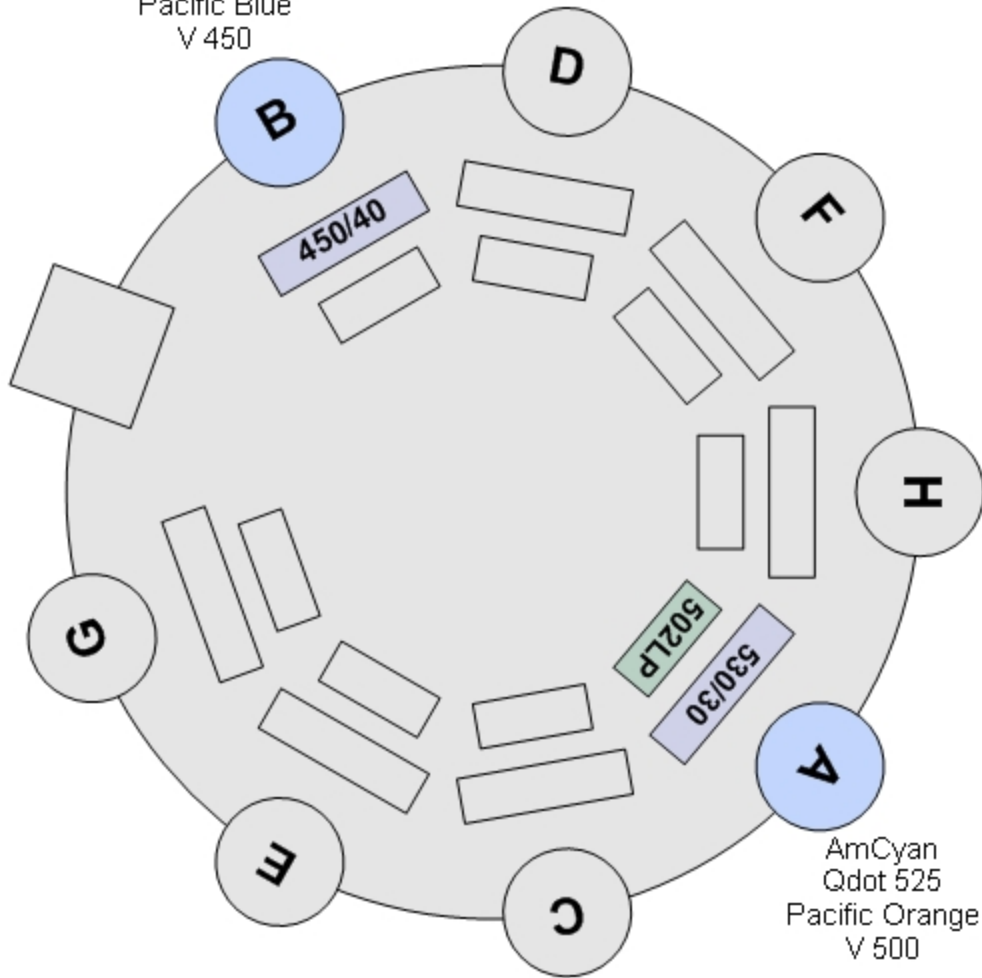

Comments: