



# VA\_5-Blue 3-Red 6-Violet

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	4/3/2017 11:32:20 AM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

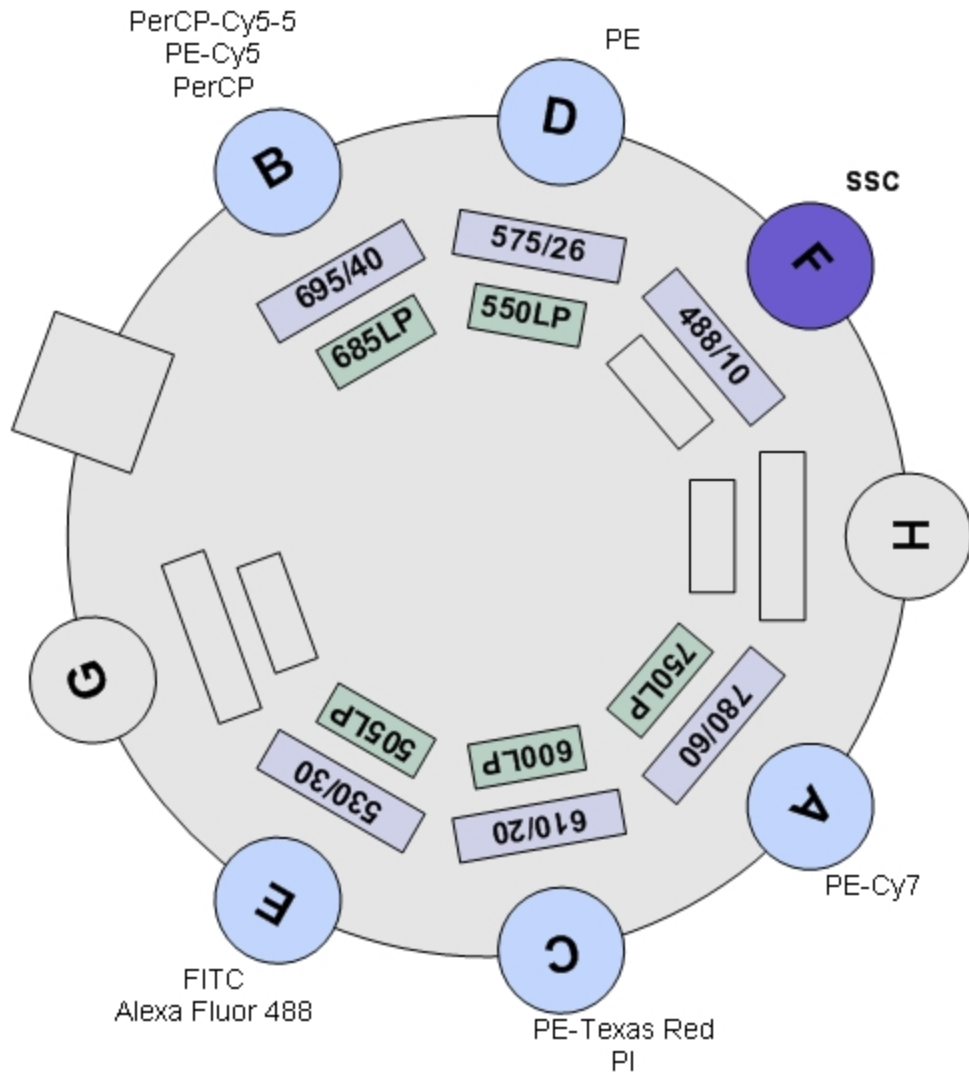

Red Laser  
(640nm)

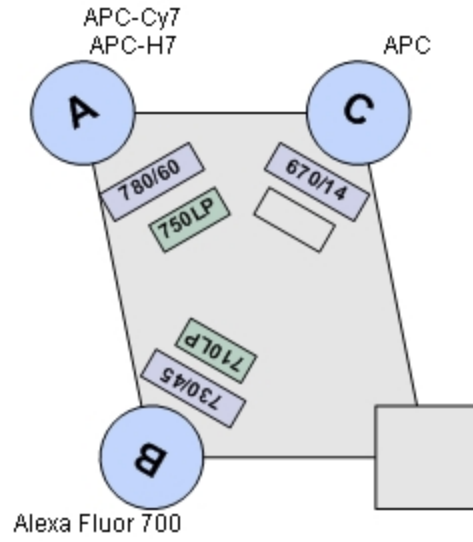

Violet Laser  
(405nm)

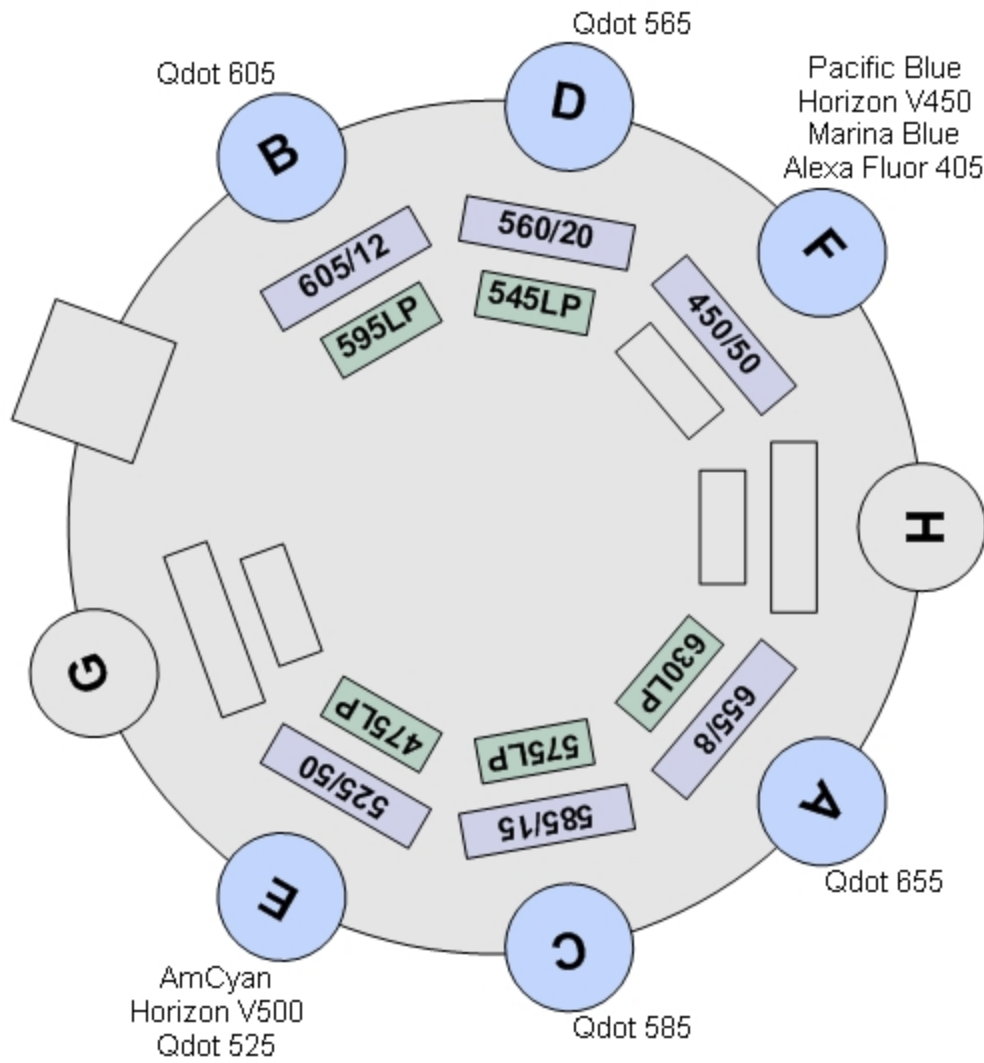

Comments: